


Nitrile Examination Gloves

Glove Plus Lite are the perfect medium weight nitrile gloves with superb chemical barrier properties and precision grip, they are the ideal everyday glove.

Manufactured in a dedicated Nitrile factory, this product is 100% Natural Rubber Latex free and is ideal for glove users who have been identified as having allergic reactions to NR Latex proteins (Type 1 reactions).

Product Key Points

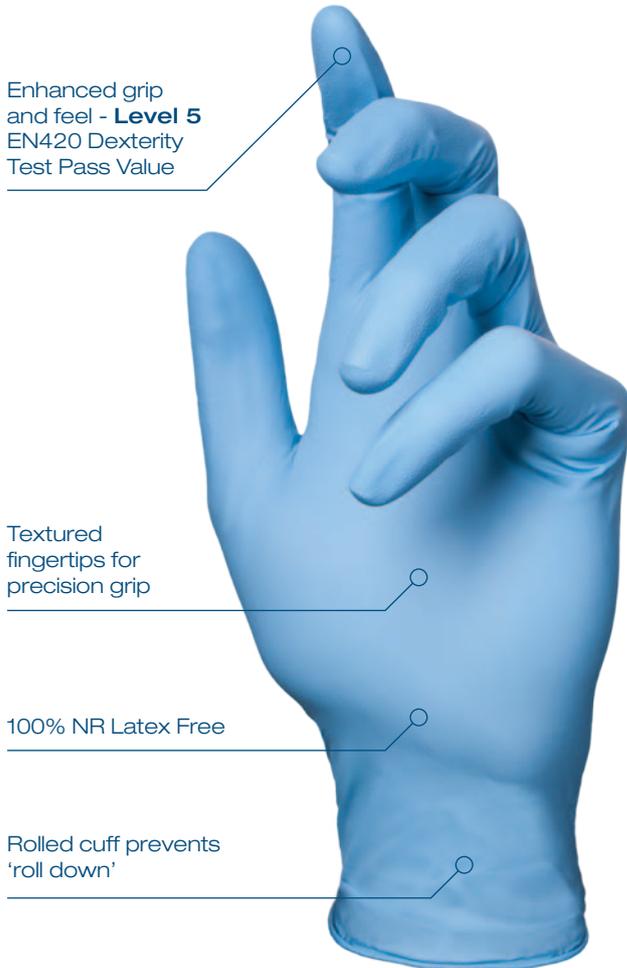

Enhanced grip and feel - **Level 5**
EN420 Dexterity
Test Pass Value

Textured
fingertips for
precision grip

100% NR Latex Free

Rolled cuff prevents
'roll down'

Product Conformance:

- EU MDD EN455 Parts 1, 2, 3 & 4.
- Manufactured in compliance to EU PPE 89/686/EEC "Protection Against Chemical Hazard".
- EN374 Parts 1, 2 & 3.
- Passed an independent test to ASTM F1671-07 "Resistance of Materials used in Protective Clothing to Penetration by Blood-Borne Pathogens" (viral test).
- EN420 Dexterity Test - Passed to the maximum Level 5.

Product Information

Type: Powder free & non-sterile.

Material: Nitrile (Synthetic Latex) - Carbocylated Acrylonitrile Butadiene.

Protein Content: 100% NR Latex free.

Powder Content: Below 2mg/g glove.

Features: Ambidextrous, Beaded Cuff, Textured fingers.

Colour: Black, Blue & Pink.

Packing: 100 gloves per dispenser, 10 dispensers per carton.

Dimensions

Glove Size	Product Code	Palm Width (mm)	Length (mm)
Extra Small	LN301	< 80	245
Small	LN302	± 80	245
Medium	LN303	± 95	245
Large	LN304	± 110	245
Extra Large	LN305	± 115	245

Thickness

Location of Thickness Measurements	Single Wall (mm)
Finger (at the tip)	0.11 ± 0.03
Palm (at centre of palm)	0.09 ± 0.03

Physical Properties

Parameters	Before Aging	After Aging
Force at Break (N)	> 7.0	6.0
Watertight AQL	0.65	N/A

Pre-Shipment Quality Inspection

Criteria	Insp Level	AQL
Dimensions	S-2	4.0
Physical Properties	S-2	4.0
1000ml Water Leak Test	G-1	0.65
Visual Inspection	S-4	4.0

Quality Assurance:

- This product is manufactured in a plant where the quality management system has been independently assessed as conforming to ISO 9001:2008 and ISO 13485:2008/AC2009.



www.glove-plus.com